


## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>4</sup> : A61M 16/00 // A61H 31/00	A1	(11) International Publication Number: WO 86/ 06969 (43) International Publication Date: 4 December 1986 (04.12.86)
(21) International Application Number: PCT/FI86/00053 (22) International Filing Date: 20 May 1986 (20.05.86) (31) Priority Application Number: 852073 (32) Priority Date: 23 May 1985 (23.05.85) (33) Priority Country: FI (71) Applicant (for all designated States except US): ETELÄ-HÄMEEN KEUHKOVAMMAYHDISTYS R.Y. [FI/FI]; Birger Jarlinkatu 4 B, SF-13100 Hämeenlinna (FI). (72) Inventor; and (75) Inventor/Applicant (for US only) : HÄKKINEN, Taisto [FI/FI]; Kaarloukatu 25, SF-13210 Hämeenlinna (FI). (74) Agent: FORSSÉN & SALOMAA OY; Uudenmaankatu 40 A, SF-00120 Helsinki (FI).		(81) Designated States: DE, GB, JP, NO, SE, SU, US.  Published With international search report. In English translation (filed in Finnish).

## (54) Title: RESPIRATION THERAPY APPARATUS

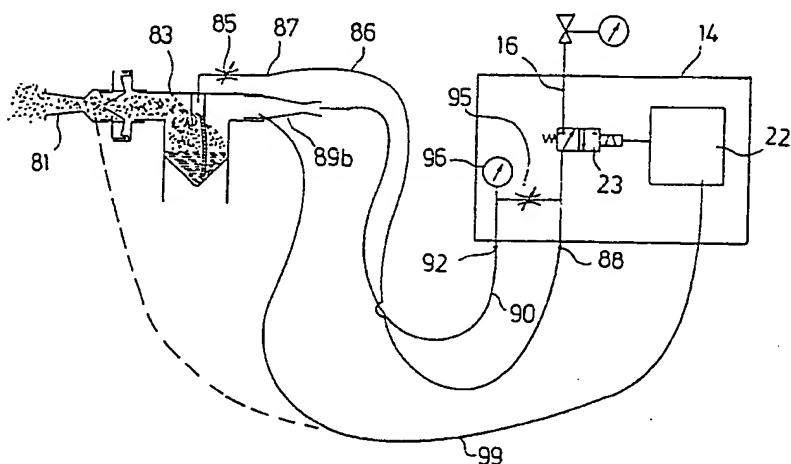

## (57) Abstract

A respiration therapy apparatus used as a drug atomizer means and/or as a so-called respirator and/or as an oxygen dispensing means. In the apparatus of the invention, administration to the patient of oxygen or air is discontinued, at the latest, when the exhalation phase starts. This has been implemented in the apparatus of the invention by employing a pressure pick-up (22) observing the differential pressure of the flow and which further provides control of an electromagnetic valve (23) which has been disposed to close and to open a pressure line (16). At commencement of the inspiration phase, the differential pressure is transmitted over a signal connection (99) to the pressure pick-up (22). The pressure pick-up (22) further controls the electromagnetic valve (23), opening the pressure line (16). The pressure pick-up (22) measuring differential pressure has been connected, as taught by the invention, over a signal connection (19, 39, 59 or 99) either to an oxygen mask, to oxygen whiskers (30), to an atomizing means (50) or to a respirator (80).

***FOR THE PURPOSES OF INFORMATION ONLY***

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GA	Gabon	MR	Mauritania
AU	Australia	GB	United Kingdom	MW	Malawi
BB	Barbados	HU	Hungary	NL	Netherlands
BE	Belgium	IT	Italy	NO	Norway
BG	Bulgaria	JP	Japan	RO	Romania
BR	Brazil	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	LI	Liechtenstein	SN	Senegal
CH	Switzerland	LK	Sri Lanka	SU	Soviet Union
CM	Cameroon	LU	Luxembourg	TD	Chad
DE	Germany, Federal Republic of	MC	Monaco	TG	Togo
DK	Denmark	MG	Madagascar	US	United States of America
FI	Finland	ML	Mali		
FR	France				

## 1   Respiration therapy apparatus

5   The present invention concerns a respiration therapy apparatus  
intended for persons suffering from respiratory diseases, for  
indisposed persons or for unconscious persons and employed as a  
respirator and/or as a drug atomizing apparatus and/or as an oxygen  
dispensing apparatus conforming to the patient's respiration, said  
10   respiration therapy apparatus comprising an oxygen or air supply  
tube connected to a regulating means, to this regulation means being  
further connected an air or oxygen line coming from an oxygen mask  
or from oxygen whiskers, and to said regulating means being con-  
15   nected an air or oxygen line coming from a drug atomizer or to  
said regulating means being connected air or oxygen lines coming  
from a respirator means comprising a mouthpiece, an exhalation  
valve, a drug atomizer and an injector, the second of said lines  
being directly connected to the injector and the first line being  
20   connected to the drug atomizer, advantageously over a regulating  
valve, for adding drug spray to the oxygen or air flow.

20   In prior art are known various kinds of respiration therapy appar-  
atus intended for persons suffering from respiratory diseases, for  
indisposed persons or for unconscious persons, the respiration  
therapy apparatus then comprising a drug atomizer, a supply pressure  
25   source communicating with the drug atomizer for conducting air or  
oxygen, an injector communicating with the drug atomizer, and  
separate regulating valves for controlling the atomizing rate of  
the drug atomizer, respectively the respiration pressure. In drug  
atomizers of prior art, the flow rate of the flowing air or oxygen  
30   is controllable. Regulating valves are known in the art through  
which the air or oxygen can be conducted. It is possible with the  
aid of electrically controlled magnetic valves, or of a magnetic  
valve controlling means, to effect control of the operating period  
of the respiration therapy apparatus in conformity with the  
35   patient's breathing rhythm; similarly, it is possible with the aid  
of separate timer means to effect regulation of the resting period

1 of the respiration therapy apparatus to conform to the patient's breathing rhythm.

Respiration therapy apparatus of prior art can be controlled with  
5 the aid of press buttons or equivalent in such manner that the operation of the respirator is paced to be appropriate for the patient, for instance specifically by pressing a button.

Likewise known in the art are respirators e.g. through the present  
10 applicant's earlier Finnish patent application No. 830059, where the respirator is used as an atomizing means. The period of operation and period of rest of the drug atomizer can be controlled with a timer means, or by pacing with finger pressure on a press  
15 button, to conform to a breathing rhythm appropriate for the particular patient, and by regulating the atomizing rate of the drug atomizer with the aid of a pressure regulator, provided with pressure gauge, inserted in the supply pressure line.

It is also previously known that an inhalation dispenser is provided  
20 with atomizing commencement time control to the purpose of selecting the time of commencement of atomizing to be advantageous for each individual patient, at the beginning of the inspiration period. This apparatus arrangement is known through the same applicant's earlier Finnish patent application No. 843769. Through the same  
25 Finnish patent application of the present applicant is also known an inhalation dispenser incorporating an inspiration flow rate control for setting at desired magnitude the inspiration flow rate advantageous for each individual patient.

30 The apparatus just discussed cannot be used in conjunction with oxygen whiskers or masks as an oxygen supplying means, nor can it serve, in this simple design, as an atomizer and respirator apparatus.

35 The drawback of oxygen supplying means of prior art, again, can be seen in the circumstance that in said oxygen also flows during the

1     exhalation period, causing unnecessary irritation of the patient's  
nostrils. It is thus understood that the patient is disturbed by  
the continuous oxygen flow, and it is understood that the detriment  
consequent on this continuous oxygen or air flow is high wasted  
5     consumption. Drug substance is also wasted, and the patient's  
environment becomes polluted.

The respirator design of the invention eliminates all drawbacks  
which have been mentioned. They have been avoided by implementing  
10     the respirator of the invention with a pressure pick-up, and so  
that to the pressure pick-up there is a signal connection. The  
signal connection has further been taken out through a connector  
from the regulating means. This pick-up indicating the pressure of  
the respiration flow is further applied to control a control valve  
15     which governs the oxygen or air flow going to the patient. The  
pick-up observes the pressure change arriving through the signal  
connection and it observes the moment when the patient commences  
his inspiration. The pick-up then acts on the control valve and  
opens the oxygen or air flow passage. Likewise, said pick-up ob-  
20     serves, through the signal connection, the commencement of the  
patient's exhalation phase, at which time the pressure pick-up  
further acts on said control valve, whereby the valve closes the  
oxygen or air passages. With this apparatus arrangement one avoids  
supply of oxygen or air or drugs to the patient during the patient's  
25     exhalation phase.

The apparatus design of the invention, which may expressly be used  
both as atomizer means, as oxygen administration means and as  
respirator, may operate at different pressure levels. It is this  
30     which enables the signal connection of the invention to be taken  
out from the control units and carried to different targets. Hereby  
the use of this apparatus design as a multi-purpose means, in  
operation at low and high pressure levels, is rendered feasible.

35     The invention is mainly characterized in that the respiration  
therapy apparatus comprises a pressure pick-up and a separate

1 connection going to the pressure pick-up arranged to close and  
open the air or oxygen supply pressure line, which over a valve  
communicates with the oxygen or air line so that when the patient's  
inspiration is taking place the pressure pick-up observes the  
5 pressure change in the inspiration air caused by the commencement  
of this inspiration phase, the pick-up having been arranged there-  
upon to open the valve similarly at commencement of the patient's  
exhalation the pressure pick-up has been arranged to control the  
valve so that the air or oxygen pressure line is closed.

10

The invention is described in greater detail in the following with  
reference to the enclosed figures.

15 In Fig. 1 is depicted a respirator according to the invention, in  
schematical presentation, and the oxygen or air tube, and the  
signal connection going to the pressure pick-up, this connection  
being attached to a face mask. Moreover, separate oxygen whiskers  
have been depicted in this figure.

20 In Fig. 2 is shown the face mask, seen from the front and in the  
direction X indicated in Fig. 1.

In Fig. 3 are shown the oxygen whiskers, attached to the patient.  
The connection to be carried to the pressure pick-up is incorporated  
25 in this figure.

In Fig. 4 is presented a respirator according to the invention,  
provided with pressure pick-up and signal connection and used as  
an atomizing means.

30

In Fig. 5 is presented a respiration therapy apparatus according  
to the invention which is used as a respirator (IPFB). The presen-  
tation is an elevational view of the apparatus.

35 In Fig. 6 is shown the apparatus of Fig. 5, in schematical presen-  
tation. The alternative placements of the other end of the signal

1 connection have been shown in this figure.

In Fig. 7 is schematically presented the connecting of a computer to the respiration therapy apparatus. Furthermore, a design is  
5 presented in which two valves have been employed.

In Fig. 1, a respiration therapy apparatus is depicted. In the figure, reference numeral 10 is used to indicate a face mask; numeral 11, to indicate the part of the mask to be placed against the face, this part being connected through an air or oxygen tube 12 to the control unit 14. The air or oxygen tube 12 is connected over a connector 13 on the mask 11 to the mask part proper, 11. The connector 15 similarly connects the tube 12 with the control unit proper, 14. The supply pressure tube, supplying oxygen or  
15 air, is indicated by reference numeral 16. This tube 16 has been connected to the control unit 14 with the connector 17. The control unit 14 comprises the oxygen or air flow operating time control 18. The apparatus of the invention comprises a signal connection 19 leading to a pressure pick-up, this connection being carried  
20 from the control unit 14 along with the tube 12 to the mask part proper 11, through the connector 20. The connector 21 connects said signal connection 19, leading to the pressure pick-up, with the control unit proper, 14. Reference numeral 22 represents schematically the pressure pick-up, or differential pressure transducer,  
25 located in the control unit 14. The current supply to the apparatus can be interrupted by operating the switch 23.

The current to the respiration therapy apparatus, and suitably also to its control unit 14, may be conveyed either from a storage  
30 battery, from a dry cell battery or from the electric mains.

The oxygen whiskers carry the reference numeral 30. These whiskers may conduct air or oxygen into the patient. The oxygen line or air line 32 branches into two lines 32a and 32b. These branches 32a  
35 and 32b are further connected to a nostril connector 31, comprising parts 33 entering the nostrils. The connection of the air or oxygen

1 line 32 to the control unit 14 is indicated with reference numeral  
35. Reference numeral 39 indicates the signal connector leading to  
the pressure pick-up. The connection of the branches 32a and 32b  
of the air or oxygen line with the nostril connector 31 is rep-  
5: resented by reference numeral 40. Connector 41 is the connection  
with the control unit 14 of the signal connection 39 leading to  
the pressure pick-up.

Fig. 3 illustrates the oxygen whiskers 30, attached to a patient.

10:

In Fig. 4 is schematically shown the use of the respiration therapy  
apparatus 10 as an atomizing means from drug dispensing. Reference  
numeral 50 indicates a drug atomizing means. To the drug atomizer  
51 is connected a supply pressure tube 52 leading to the drug  
15 atomizer. Control of atomizing rate takes place through the valve  
53. Reference numeral 59 represents the connection going to the  
pressure pick-up 22. The pick-up 22 in its turn controls an  
electromagnetic valve 23, its opening and closing. Through this  
valve 23, the oxygen or air is carried along the supply pressure  
20 tube 52. The conical connector 60 of the signal connection attaches  
to the drug atomizer 51. The air or oxygen supply pressure line 16  
goes to the valve 23. In this line 16 is incorporated a supply  
pressure valve 16a and, in association therewith, a supply pressure  
gauge 16b. The drug atomizer 51 is provided with a mouthpiece 24,  
25 through which the flow enters the patient. The signal connection  
59 leading to the pressure pick-up has been connected to the conical  
connector 60 on the drug atomizer 51. The operation of the unit is  
such that when the patient is inhaling through the mouthpiece 24,  
there is a flow through the conical connector 60, whereby the  
30 pressure falls in this connector 60. This pressure drop is observed  
by the pressure pick-up 22, and the pressure drop is transmitted  
through the signal connection 59 to the pick-up 22. The signal  
connection is appropriately a length of plastic tubing. The pick-  
up 22 transmits the information, controlling the electromagnetic  
35 valve 23 and opening a connection from the supply pressure line 16  
to the supply pressure tube 52 going to the drug atomizer 51.



1 Hereby an atomized drug spray will in the course of the patient's  
inspiration be admixed to the air entering through the conical  
connector 60, said atomized spray being produced by the air or  
oxygen flow to the drug atomizer 51 taking place along the supply  
5 pressure tube 52. The control unit 14 may furthermore comprise a  
means by which the maximum time of drug atomizing is regulated. If  
the inspiration phase exceeds this maximum time, said maximum time  
controller shuts off the communication from the pressure line 16  
to the supply pressure tube 52 and the atomizing process is inter-  
10 rupted. In any other case, when the patient commences exhalation  
through the mouthpiece 24, the pressure in 59 increases, and this  
pressure rise is observed by the pressure pick-up 22, which then  
controls the electromagnetic valve 23 and shuts off the connection  
between the supply passage 16 and the supply pressure tube 52, the  
15 atomizing process ceasing forthwith.

In Fig. 5 is illustrated, in elevational view, the use of respira-  
tion therapy apparatus as a true respirator. The respirator, now  
indicated with reference numeral 80, comprises a mouthpiece 81, an  
20 exhalation valve 82, an atomizer 83. From the control unit 14, a  
supply pressure line 86 for oxygen or air runs over the connector  
87 to the atomizer 85. The supply pressure line 86 is connected  
over the connector 88 with the control unit 14. The flow connector  
90 is connected over the connector 92 with the control unit 14,  
25 and over the connector 91 with the injector 89, i.e., with its  
injector nozzle 89a. The injector 89 is further joined with the  
body of the atomizer 83. The control arrangement of the invention  
is furthermore composed of a pressure pick-up 22, appropriately  
located in the control unit 14. From the pressure pick-up 22 and  
30 from the control valve 14, the signal connection 99 leads either  
to the mouthpiece 81 or to the atomizing means 83, and in that  
case suitably to its conical connector. The control unit 14 moreover  
comprises a timer means 94 for the time of operation of the atomizer  
and a respiration pressure regulator, suitably a regulating valve  
35 95. The control unit 14 further comprises a gauge 96 indicating  
the respiration pressure. The gauge 96 indicating the respiration

1 pressure is connected, as shown in Fig. 6, to the flow connector  
90. The respiration pressure regulating valve 95 may be connected  
either directly to the flow connector 90 or to the line leading to  
said connector 90. When the patient's inspiration is taking place,  
5 the pressure pick-up 22 through the signal connection 99 observes  
the change of pressure and controls the electromagnetic valve 23,  
as in the embodiment of Fig. 4. When the patient's exhalation  
commences, the pressure rises at the signal connector 99. The  
pressure pick-up 22 observes this change and controls the electro-  
10 magnetic valve 23, shutting the pressure line off. The signal  
connection 99 may be connected either to the conical connector 89b  
of the atomizer 83 or directly to the mouthpiece 81 going to the  
patient.

15 The pressure pick-up 22 may also be disposed so that it is located  
directly in the oxygen or air flow entering the patient. In that  
case, an electrical signal is conducted from the pressure pick-up  
22 along the signal connection to the control unit 14 and further  
to the electromagnetic valve 23. Most appropriately, however, the  
20 signal connection is a flexible tube and the pressure pick-up has  
been disposed to be located expressly in the control unit 14. The  
changes of pressure are then transmitted along the hollow tube to  
the pressure pick-up 22. The oxygen and air lines, or connectors,  
are suitably pieces of plastic tubing consisting of some plastic  
25 material.

In Fig. 7 is presented a design in which in addition to the valve  
23 also another valve 98 is employed, this valve too, appropriately,  
an electromagnetic valve. The valve 98 has been placed in the flow  
30 connector 90 or in the control unit 14 in such manner that it  
communicates with the line 90. The pressure pick-up 22 controls  
the valve 98, either directly or over electronic circuitry 97; the  
latter may suitably consist of a timer means. In that case it  
becomes possible to time the opening of the line 90 and the opening  
35 of the line 86 to the pressure line 16 to be as desired, and favour-  
able from the therapeutic point of view.

1 In Fig. 7 has also been shown the connecting of a computer, suitably  
a micro-processor, to the respiration therapy apparatus of the  
invention. The computer or equivalent has been indicated with  
reference numeral 100. The computer is by one or several cables  
5 connected to the respiration therapy apparatus of the invention.  
This signal line between the computer and the respiration therapy  
apparatus has been denoted, in general, with reference numeral  
110. The computer has been arranged, with the aid of a programme  
stored therein, to place the respiration therapy apparatus of the  
10 invention into operation and out of operation. The computer 100  
may simultaneously control one or several respiration therapy  
apparatuses. In the latter case one person is enabled to program  
the therapy schedules individually for each patient. The computer  
may equally be programmed to operate the respiration therapy appar-  
15 atus of the invention in such manner that with the aid of a pro-  
gramme stored in the computer's memory are controlled the thera-  
peutic variables of the respiration therapy apparatus, such as  
respiration pressure, drug atomizing, etc. A data line, or data  
lines, carried in a suitable manner from the computer, and which  
20 have been denoted in general with reference numeral 110, are  
connected to the control unit 14. In the figure has been depicted  
a computer 100, connected over a data line, or data lines, 110 to  
a respiration therapy apparatus 80 according to the invention.

25 The computer 100 may be arranged to control the valve 98, which is  
suitably an electromagnetic valve. The computer 100 may be arranged  
to control either separately the valves 23 and 98, or to control  
both in dependence of each other, as specified in each case in the  
programme that has been stored. The computer 100 may be made to  
30 control the valve 98 over supply electronics 97, suitably a timer  
means. The computer 100 has been disposed to control the valve 98  
and/or the valve 23 so that the connection from the supply pressure  
line 16 to the flow connector 90 and/or the flow connector 86 is  
opened.

## Claims

1. A respiration therapy apparatus intended for persons suffering from respiratory diseases, for indisposed persons or for unconscious persons and which is used as a respirator (IPPB) and/or as a drug atomizing means and/or as an oxygen dispensing means conforming to the patient's respiration, said respiration therapy apparatus comprising an air or oxygen supply pressure tube (16) connected to a control unit (14), to said control unit (14) being further connected an air or oxygen line (12,32) coming from an oxygen mask (10) or from oxygen whiskers (30), or to said control unit (14) being connected an oxygen or air line (52) coming from a drug atomizer (51), or to said control unit (14) being associated oxygen or air lines (86,90) coming from a respirator (80) comprising a mouthpiece (81), an exhalation valve (82), a drug atomizer (83) and an injector (89), whereof the second line (90) is connected directly to the injector (89) and the first line (86) is connected to the drug atomizer (83), preferentially over a regulating valve (85), for adding atomized drug spray to the oxygen or air flow; the respiration therapy apparatus comprises a pressure pick-up (22) and a separate connection leading to the pressure pick-up and arranged to close and open the air or oxygen supply pressure line (16), which over a valve communicates with the oxygen or air line (12 or 32 or 52 or 90 and 86) so that when the patient's inspiration is taking place the pressure pick-up (22) observes the change of pressure in the inspiration air caused by the commencement of this inspiration phase, whereat the pressure pick-up (22) has been arranged to open the valve and, respectively, at commencement of the patient's exhalation the pressure pick-up (22) has been arranged to control the valve so that the air or oxygen pressure line (16) is closed, characterized in that the control unit (14) comprises a timing means (94) which regulates the oxygen or air flow coming to the atomizer (83,51), to the oxygen whiskers (30) or to the oxygen mask (10), and that the signal or control variable coming from the pressure pick-up (22) has been arranged, counted from commencement of the inspiration phase, to start the count of a timing means

(94) provided in the control unit (14), in said timing means (94) having been pre-set that maximum time during which the valve is open and admits the air or oxygen flow to the oxygen whiskers (30) or to the oxygen mask (10) or to the atomizer means (50) or to the respirator (80).

2. Respiration therapy apparatus according to claim 1, characterized in that the control unit (14) comprises, in addition to a first valve (23), also a second valve (98), which is advantageously an electromagnetic valve, and which communicates with the oxygen or air line, and that the pressure pick-up (22) is arranged either directly or over electronic circuitry, most preferably a timing means (97), to control the valve (98), whereby the opening of the oxygen and/or air line going to the patient from the control unit (14) to communicate with the pressure line (16) can be timed to be as desired and appropriate from a therapeutic point of view.

3. Apparatus according to claim 1 or 2, characterized in that a signal connection has been carried out from the control unit (14) and has by one end been connected to the pressure pick-up (22) and by its other end connected to a therapy apparatus consistent with each therapeutic measure.

4. Apparatus according to claim 1, 2 or 3, characterized in that the pressure pick-up (22) has been disposed to be located in the control unit (14).

5. Apparatus according to any one of claims 1-4, characterized in that to the pressure pick-up (22) leads a connection (19) which is connected to an oxygen mask (10) at its other end.

6. Apparatus according to any one of claims 1-4, characterized in that to the pressure pick-up (22) has been connected a connector (39) which is further connected to oxygen whiskers (30).

7. Apparatus according to any one of claims 1-4, characterized in

that with the pressure pick-up (22) is connected a connector (59) which has further been connected to a conical connector (60) on an atomizer (51).

8. Apparatus according to any one claims 1-4, characterized in that with the pressure pick-up (22) is associated a connector (92) which is by one end connected to the end adjacent to the atomizing means (83) of the injector (89) in a respirator (80) or in the vicinity of the mouthpiece (89) of the respirator (89) or to the mouthpiece (81) itself.

9. Apparatus according to any one of the preceding claims, characterized in that the pressure pick-up (22) has been disposed to control a valve (23), which is an electromagnetic valve.

10. Apparatus according to any one of the preceding claims, characterized in that the connection (99,59) coming from the pressure pick-up (22) connects by its other end with a part (89,60) having conical cross-section.

11. Apparatus according to claim 1 or 2, characterized in that the pressure pick-up (22) has been disposed to be located directly in the oxygen or air flow entering the patient, and that from the pressure pick-up (22) an electrical signal has been conducted along a signal connection to the control unit (14) and further to the electromagnetic valve (23).

12. Apparatus according to any one of the preceding claims, characterized in that the pressure pick-up (22) has been disposed to control either directly a valve (98) placed in a flow connector (90) or a valve (98) disposed in the control unit (14) and connected to the flow connector (90).

13. Apparatus according to any one of the preceding claims, characterized in that a computer (100) has been disposed over a data line, or data lines, (110) to control the respiration therapy

apparatus.

14. Apparatus according to the preceding claim, characterized in that the data line, or data lines (110) has/have been connected directly to the control unit (14).

15. Apparatus according to any one of the preceding claims, characterized in that the computer (100) has been disposed to control the valve (98) and/or the valve (23) so that a connection is opened or closed from the supply pressure line (16) to the flow connector (90) and/or to the flow connector (86).




FIG. 2



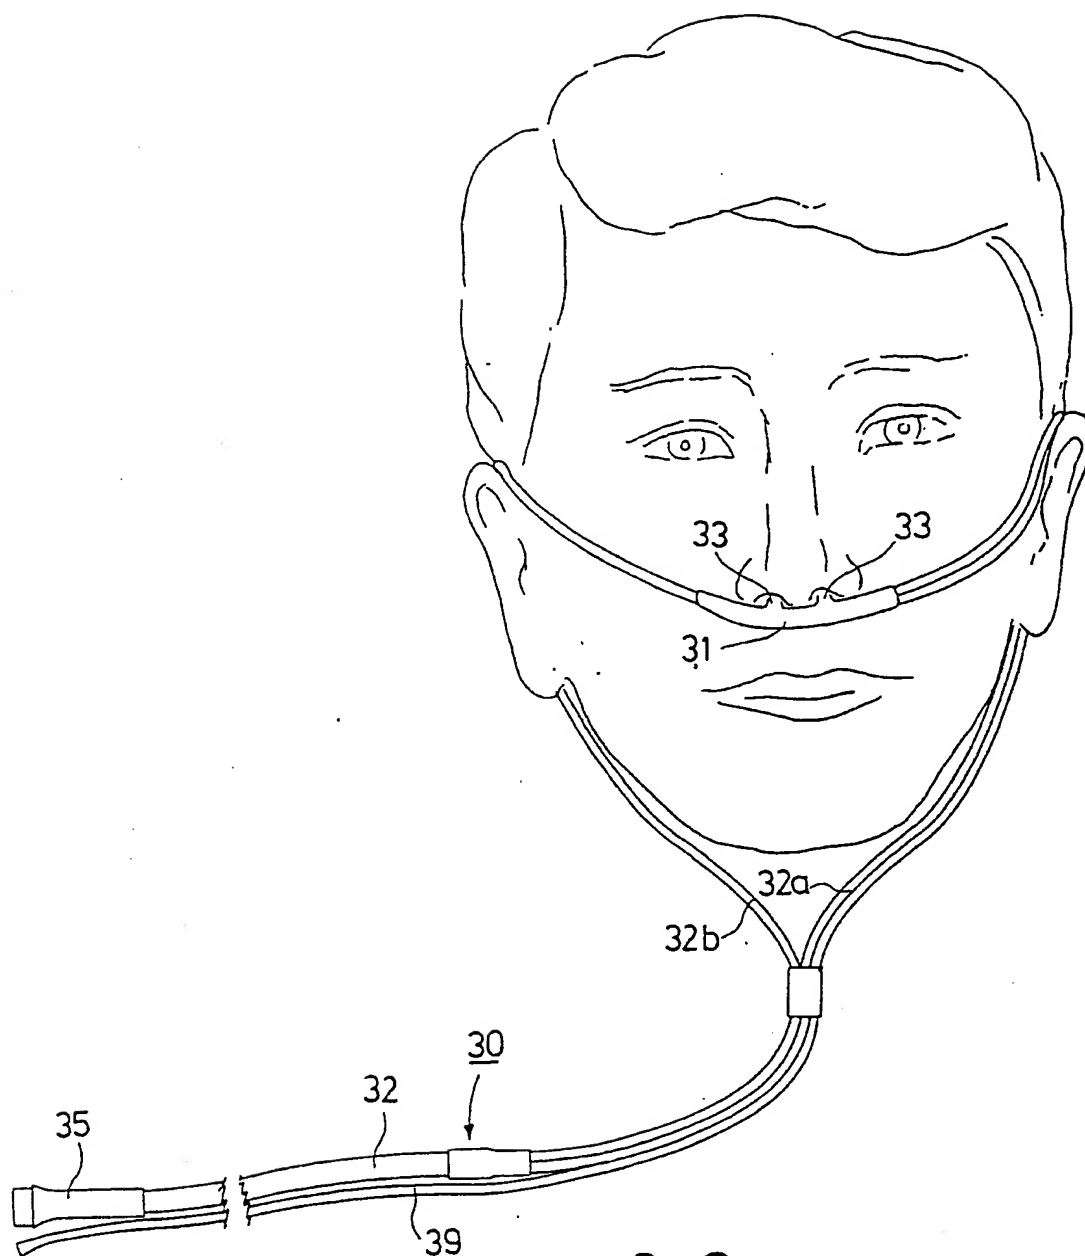


FIG. 3

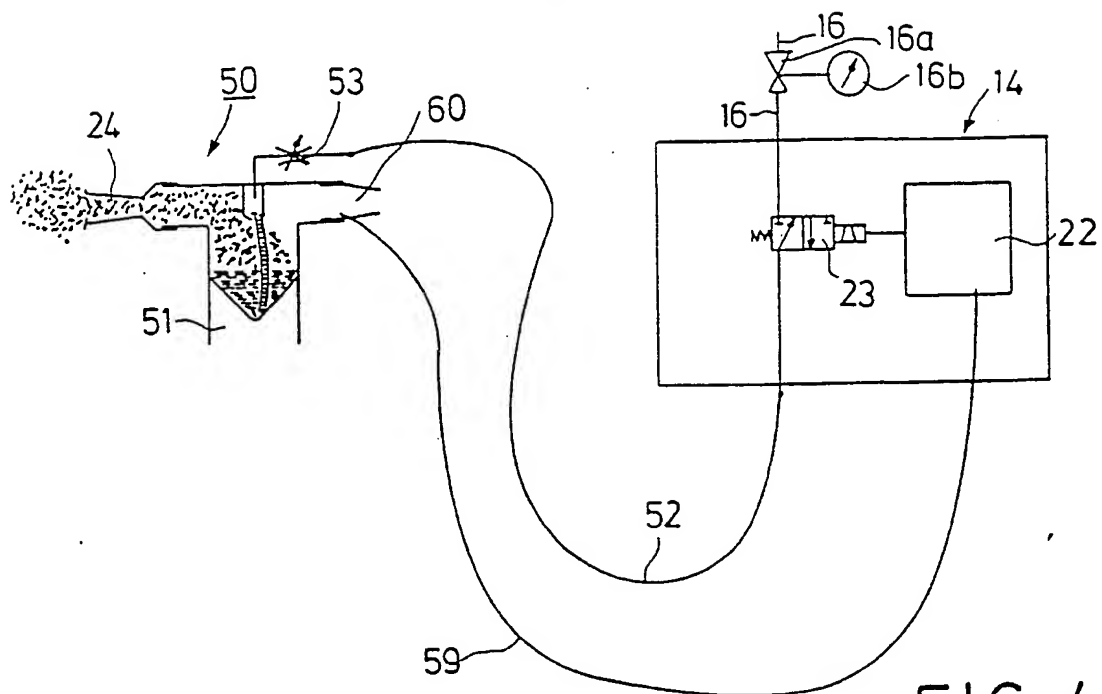


FIG. 4

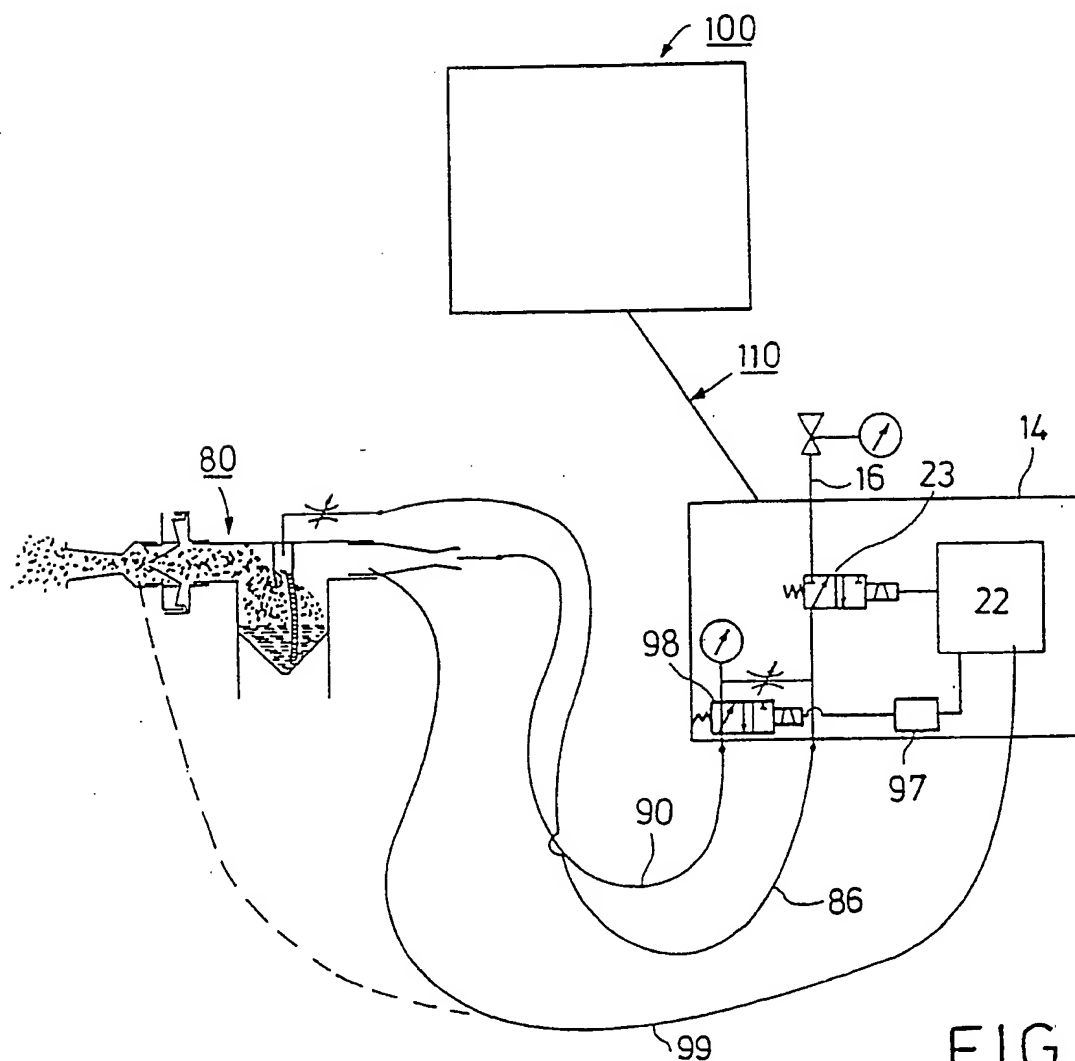


FIG. 7

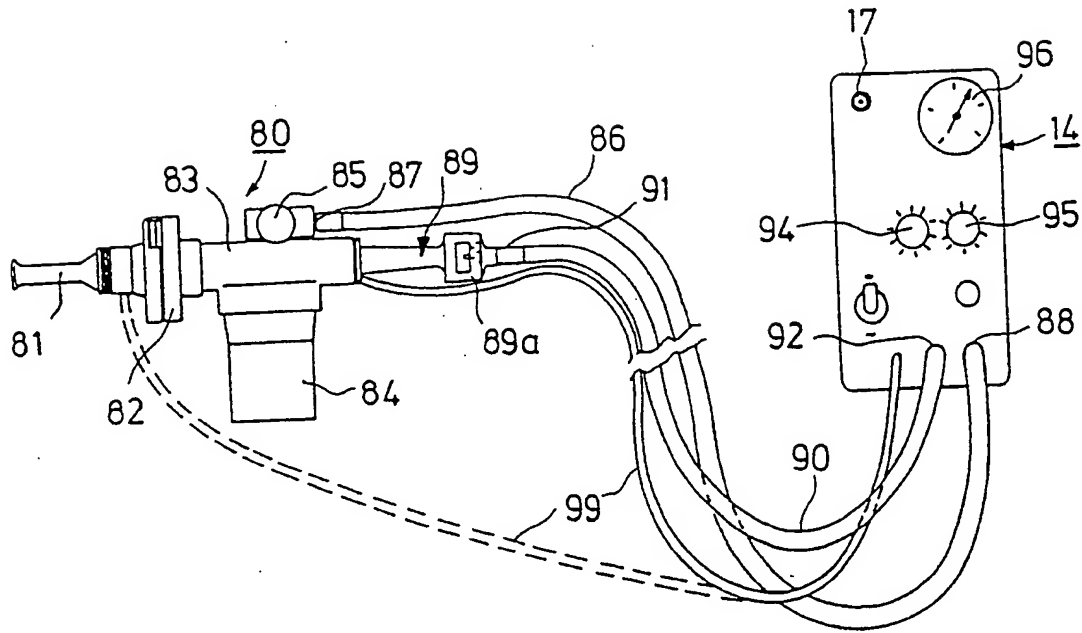


FIG. 5

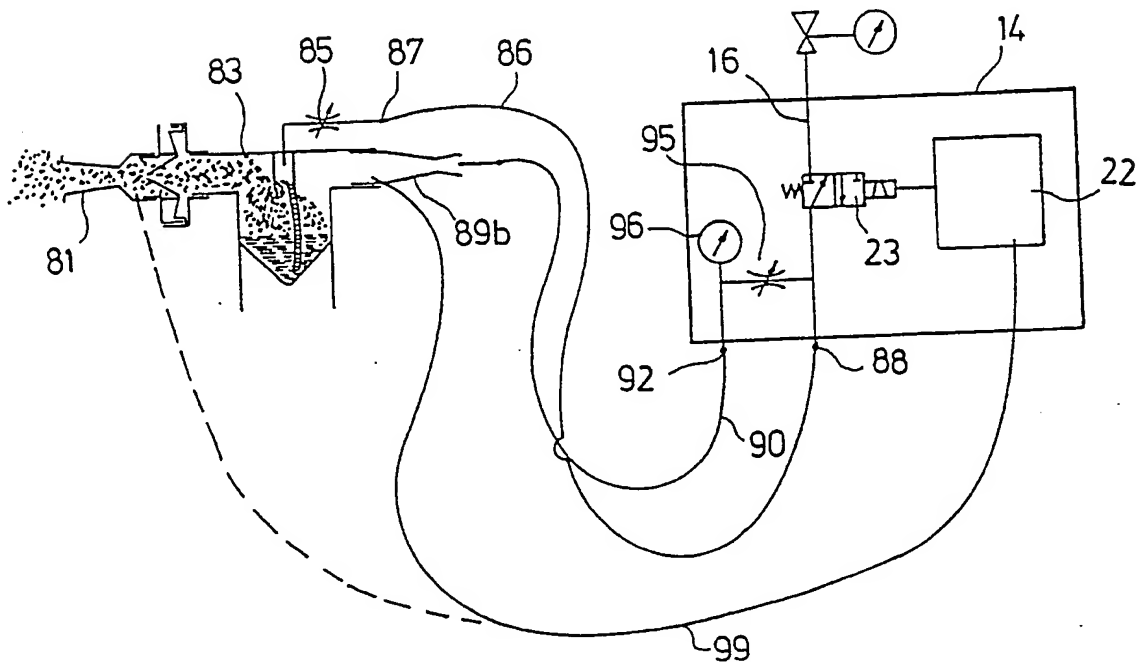



FIG. 6

# INTERNATIONAL SEARCH REPORT

International Application No

PCT/FI86/00053

<b>I. CLASSIFICATION OF SUBJECT MATTER</b> (If several classification symbols apply, indicate all) *		
According to International Patent Classification (IPC) or to both National Classification and IPC <sup>4</sup>		
A 61 M 16/00 // A 61 H 31/00		
<b>II. FIELDS SEARCHED</b>		
Minimum Documentation Searched <sup>7</sup>		
Classification System	Classification Symbols	
IPC 4 US Cl	A 61 H 31/00-/02; A 61 M 16/00, /10-/20 128:145.5-145.8, 198-205	
Documentation Searched other than Minimum Documentation to the Extent that such Documents are Included in the Fields Searched *		
SE, NO, DK, FI classes as above		
<b>III. DOCUMENTS CONSIDERED TO BE RELEVANT <sup>1</sup></b>		
Category *	Citation of Document, <sup>11</sup> with indication, where appropriate, of the relevant passages <sup>12</sup>	Relevant to Claim No. <sup>13</sup>
X	SE, B, 386 366 (G.E. SMYTHE ET AL) 9 August 1976 & NL, 7211141 GB, 1288019 FR, 2149580 DE, 2238928 US, 3921628	1-5, 9-12
X	SE, B, 434 597 (E. SCHWANBOM ET AL) 6 August 1984 & NL, 7807874 FR, 2406436 GB, 2007101 DE, 2746924 JP, 54068095 US, 4211221 CH, 635246 SE, 7810852	1-5, 9-12
A	DE, A, 2 124 446 (L. HELM ET AL) 23 December 1971	1-4, 7-12
*.../...		
<div style="display: flex; justify-content: space-between;"> <div style="width: 45%;"> <p>* Special categories of cited documents: <sup>10</sup></p> <p>"A" document defining the general state of the art which is not considered to be of particular relevance</p> <p>"E" earlier document but published on or after the international filing date</p> <p>"L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)</p> <p>"O" document referring to an oral disclosure, use, exhibition or other means</p> <p>"P" document published prior to the international filing date but later than the priority date claimed</p> </div> <div style="width: 45%;"> <p>"T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention</p> <p>"X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step</p> <p>"Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art</p> <p>"A" document member of the same patent family</p> </div> </div>		
<b>IV. CERTIFICATION</b>		
Date of the Actual Completion of the International Search	Date of Mailing of this International Search Report	
1986-09-15	1986 -09- 16	
International Searching Authority	Signature of Authorized Officer	
Swedish Patent Office	 Lelf Karnsäter	

## III. DOCUMENTS CONSIDERED TO BE RELEVANT (CONTINUED FROM THE SECOND SHEET)

Category *	Citation of Document, with indication, where appropriate, of the relevant passages	Relevant to Claim No
A	GB, A, 1 158 124 (J.E. FINAN) 16 July 1969	1, 6, 12
X	US, A, 2 830 580 (M. SAKLAD ET AL) 15 April 1958	1-5, 9-15
A	US, A, 4 060 078 (F.M. BIRD) 29 November 1977	1-5, 9-12
A	US, A, 4 396 015 (R.J. JOHNSON) 2 August 1983	1,7-10
A	Medical and Biological Engineering, May 1973, pages 262-267, "computer control of respiration and anaesthesia" by J.R. Coles, W.A. Brown and D.G. Lampard.	1,13-15

**This Page is Inserted by IFW Indexing and Scanning  
Operations and is not part of the Official Record**

**BEST AVAILABLE IMAGES**

Defective images within this document are accurate representations of the original documents submitted by the applicant:

Defects in the images include but are not limited to the items checked:

- ☒ **BLACK BORDERS**
- ☐ **IMAGE CUT OFF AT TOP, BOTTOM OR SIDES**
- ☐ **FADED TEXT OR DRAWING**
- ☐ **BLURRED OR ILLEGIBLE TEXT OR DRAWING**
- ☐ **SKEWED/SLANTED IMAGES**
- ☐ **COLOR OR BLACK AND WHITE PHOTOGRAPHS**
- ☐ **GRAY SCALE DOCUMENTS**
- ☐ **LINES OR MARKS ON ORIGINAL DOCUMENT**
- ☐ **REFERENCE(S) OR EXHIBIT(S) SUBMITTED ARE POOR QUALITY**
- ☐ **OTHER:** \_\_\_\_\_

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning these documents will not correct the image problems checked, please do not report these problems to the IFW Image Problem Mailbox.**